
Addendum: User Guide AutoPulse® Resuscitation System Model 100 with Defibrillator Interface

3.5 Periodic Electrocardiogram (ECG) Monitoring and/or Defibrillation

When the AutoPulse is used in conjunction with defibrillators or with other therapeutic devices that monitor an ECG signal, interruption of the compression cycles is required to avoid ECG motion artifact associated with mechanical chest compressions.

3.9 Defibrillator Interface

Note: Follow all Warnings and Cautions for the AutoPulse and ZOLL Defibrillators. For more information, please refer to the AutoPulse User Guide and the appropriate ZOLL Operator's Guide.

To improve cable management, connectors on the AutoPulse may be used as a pass-through connector only when used in conjunction with the following ZOLL Defibrillators and Electrodes which have been tested with the AutoPulse.

Compatible ZOLL Defibrillators

M Series®

R Series™

E Series®

Compatible ZOLL Electrodes

stat•padzII® Electrodes

CPR-D•padz™ Electrode

When connections are complete, the ECG signal will travel from the Electrodes, passing through the AutoPulse Platform and continue onto the Defibrillator. Similarly, a defibrillation shock can be sent from the Defibrillator, passing through the AutoPulse Platform, and continuing onto the Electrodes. To use this function, both the Electrodes and the Defibrillator must be connected to the AutoPulse.

3.9.1 Making the Connections

The Connector Site is located at the top of the AutoPulse next to the Battery bay (see Figure 3-23 below).

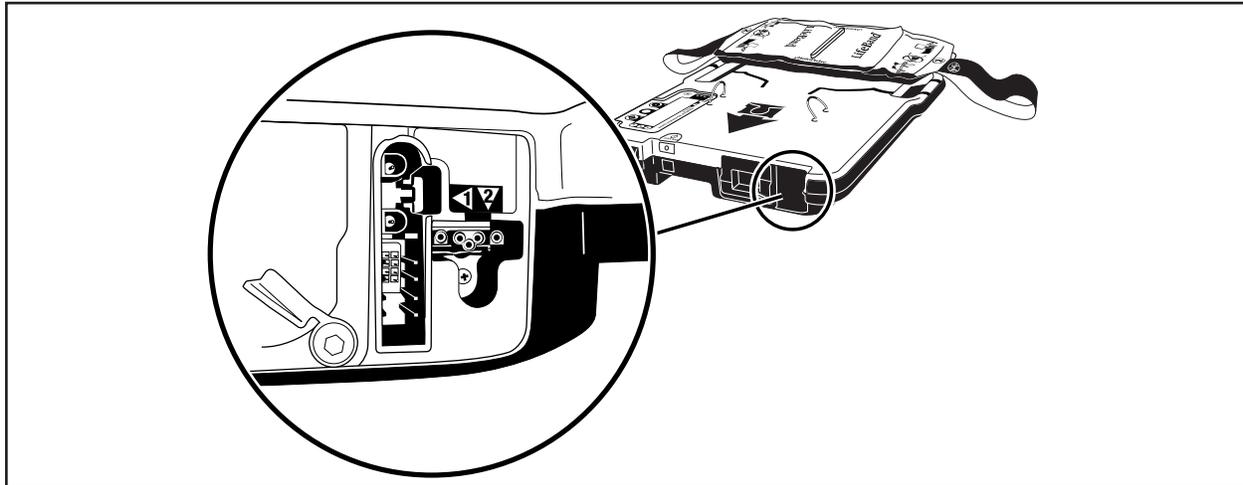


Figure 3-23 AutoPulse Connector Site

3.9.1.1 Connecting the Electrodes to the AutoPulse

First, connect the Electrodes to the AutoPulse by plugging them into the Connector Site on the AutoPulse Platform as shown in Figure 3-24 below. The Electrodes Connector should be firmly seated into the Connector Site.

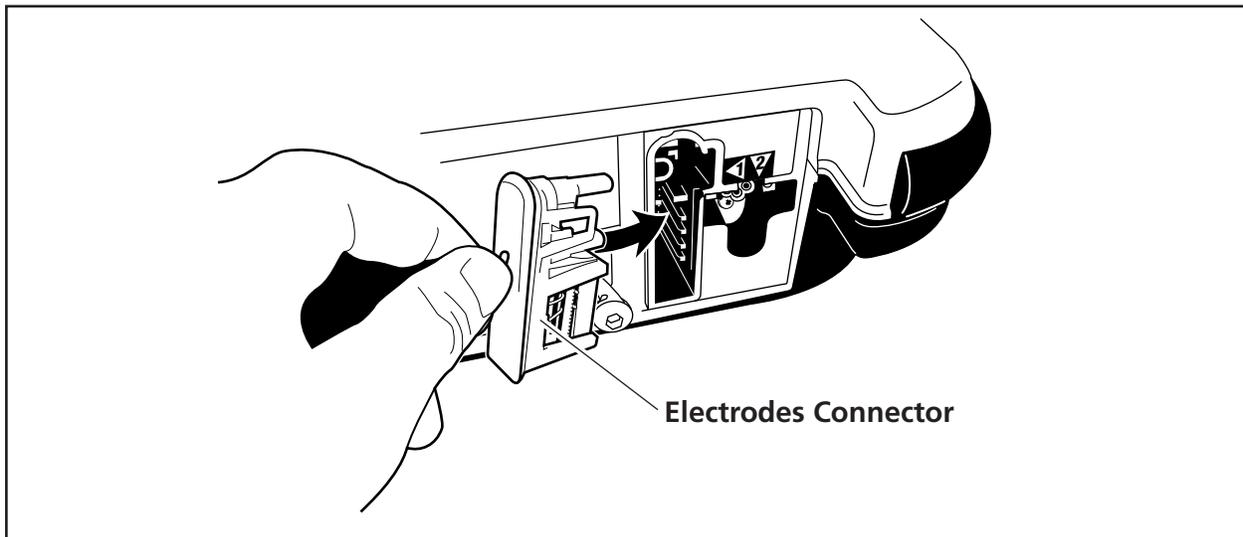


Figure 3-24 Connecting the Electrodes to the AutoPulse

3.9.1.2 Connecting the Defibrillator to the AutoPulse

Then, connect the Defibrillator to the AutoPulse as shown in Figure 3-25 below. The Defibrillator Cable should be firmly seated into the Connector Site.

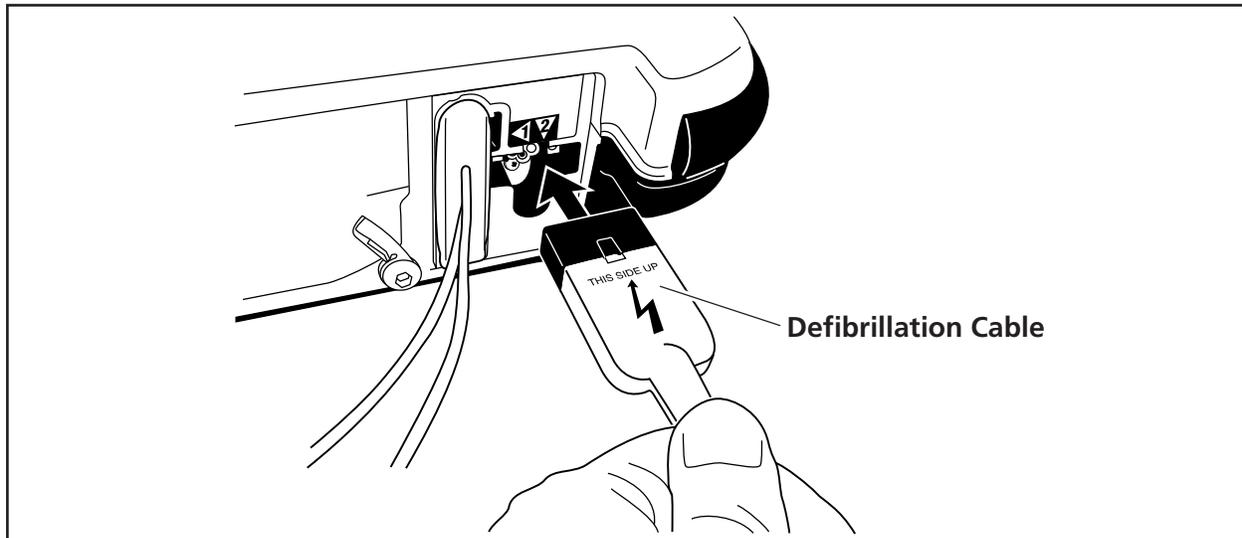


Figure 3-25 Connecting the Defibrillation Cable to the AutoPulse

4.2 Cleaning the AutoPulse

Follow the cleaning instructions listed in the AutoPulse User Guide, using the following recommended cleaning agents:

- 70% Isopropyl Alcohol
- Chlorine Bleach Solution (30ml/l water)
- Super Sani Cloths

Note: Do not use corrosive cleaning agents on the AutoPulse or Connector Site. Do not attempt to sterilize or autoclave the AutoPulse.

After cleaning, gently rinse the Connector Site with water and allow to completely dry prior to being placed back in service.

5.4 Troubleshooting Defibrillator Connections

For troubleshooting these connections, follow the prompts that appear on the Defibrillator's screen. For further assistance, please refer to the AutoPulse User Guide and the appropriate ZOLL Operator's Guide.

In the event that a connection issue cannot be resolved, unplug the Defibrillation Cable and the Electrodes from the AutoPulse and connect them directly together as shown.

5.4.1 M-Series and E-Series

The MFC and the Electrodes can be connected directly as shown in figure 5-7 below.

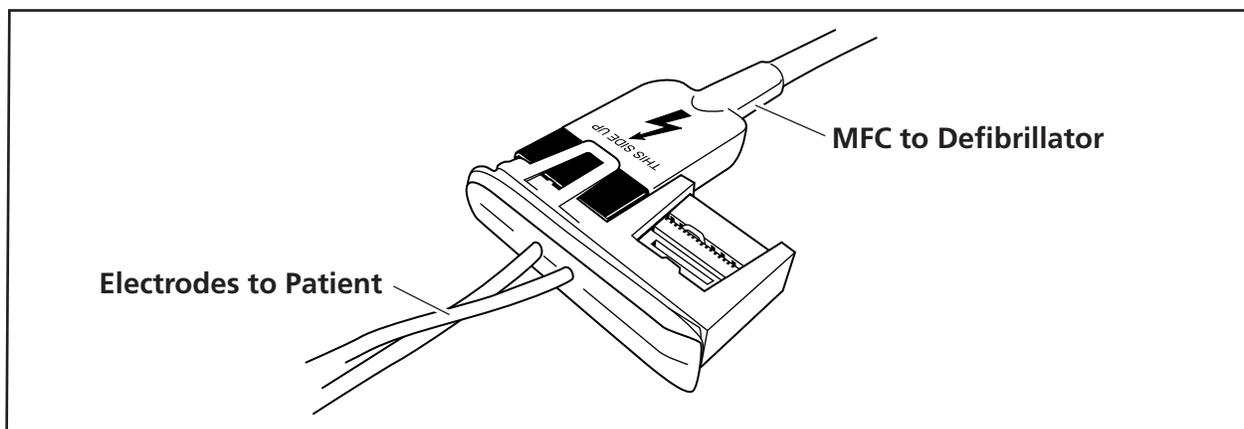


Figure 5-7 Connecting Electrodes to MFC directly

5.4.2 R-Series

The OSC and the Electrodes can be connected directly as shown in figure 5-8 below.

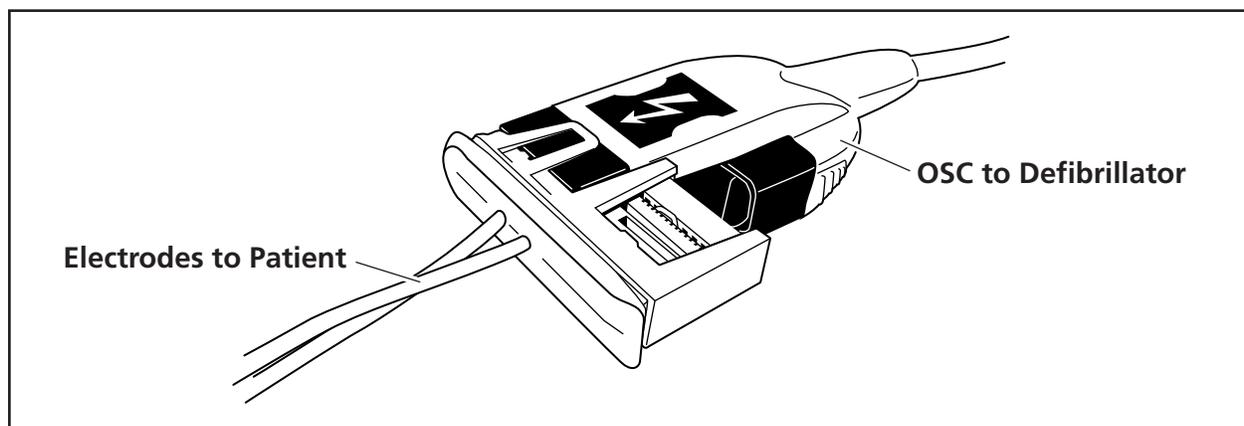


Figure 5-8 Connecting Electrodes to OSC directly